




Inhaler Resistance Range

- High**
- Med High**
- Medium**
- Med Low**
- Low**
- pMDI**

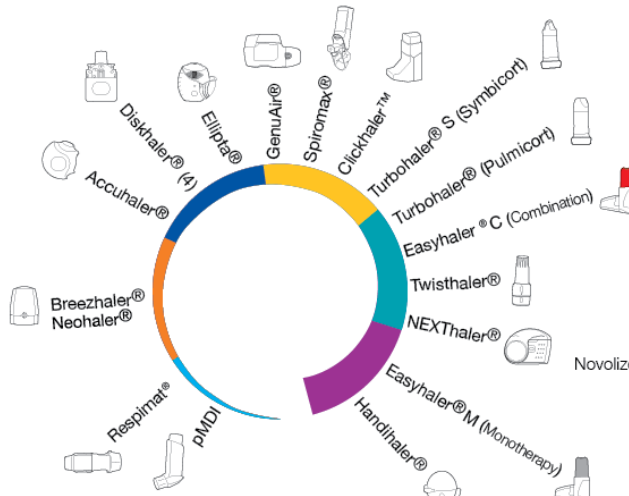

International

- Handihaler®
- Easyhaler®
- NEXThaler®
- Twisthaler®
- Turbuhaler®
- Turbuhaler®, Flexhaler®
- Clickhaler™
- RespiClick®, Spiromax®
- Novolizer®, Genuair®, Pressair®
- Ellipta®
- Diskhaler®
- Diskus®
- Breezhaler®, Aerolizer®
- Neohaler®
- Respimat®

Alliance Tech Medical
 PO Box 6024, Granbury, TX 76049
 1.800.848.8923 / 817.326.6357 Fax: 817.326.2182
 www.alliancetekmedical.com

©Copyright 2016 Clement Clarke International Ltd.
 Part no. 3109306 Issue no. 3 Jan 17



Additional Information Regarding US Inhaler Products						
Resistance Range	pMDI	Low	Med Low	Medium	Med High	High
Devices	HFA, Respimat	N/A	Ellipta Diskus	Pressair	Flexhaler Twisthaler	Handihaler
Specific Products	Advair HFA Albuterol HFA (ProAir, Proventil, Ventolin) Alvesco HFA Asmanex HFA Atrovent HFA Bevespi Aerosphere Dulera HFA Fluticasone HFA Symbicort HFA Xopenex HFA Combivent Respimat Spiriva Respimat Striverdi Respimat	Qvar Redihaler	Anoro Ellipta Arnuity Ellipta Breo Ellipta Incruse Ellipta Trelegy Ellipta Serevent Diskus	Tudorza PressAir	Pulmicort Flexhaler Asmanex Twisthaler	Spiriva Handihaler

Inspiratory flows in the range of 15 L/min to 120 L/min can be measured. The In-Check Dial is accurate to +/- 10% or 10 L/min (whichever is greater). Performance Accuracy: Accuracy +/- 10% or 10 L/min (whichever is the greater) and repeatability of +/- 5 L/min.

